



ANALIZA BIAŁEK



100004731

Laboratory of Analysis

Client: ep-company
Order number: 100004731
Name: EURO-PHARMACIES BOLDENONE UNDECYLENATE
Number of samples: 1 vial

Batch number: -----
Recive date: 2024-02-19
Start date: 2024-02-26
End date: 2024-02-28

Sample identification

Substance	Method of taking a sample	Form
Boldenone Undecylenate	Sample provided by customer	Transparent liquid in a glass vial

Results

Substance	Sample name	Content	Purity
Boldenone Undecylenate	EURO-PHARMACIES BOLDENONE UNDECYLENATE 200MG/ML	194,32mg/ml	-----

Research comment

The test sample was applied in the amount of 3 µl to the BioBasic 8 Thermo Scientific column. During the analysis with the method a linear gradient in the solutions of H2O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peak of the sought substance appeared. Its concentration, when compared to the reference chromatogram, is 194,32mg/ml. The measurement error is + - 1mg. The actual state of the sample sent before the test is presented on the photo below

Photo of the test sample



Password

A7DB3E9D

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajac




ANALIZA BIAŁEK



100004731

Chromatogram

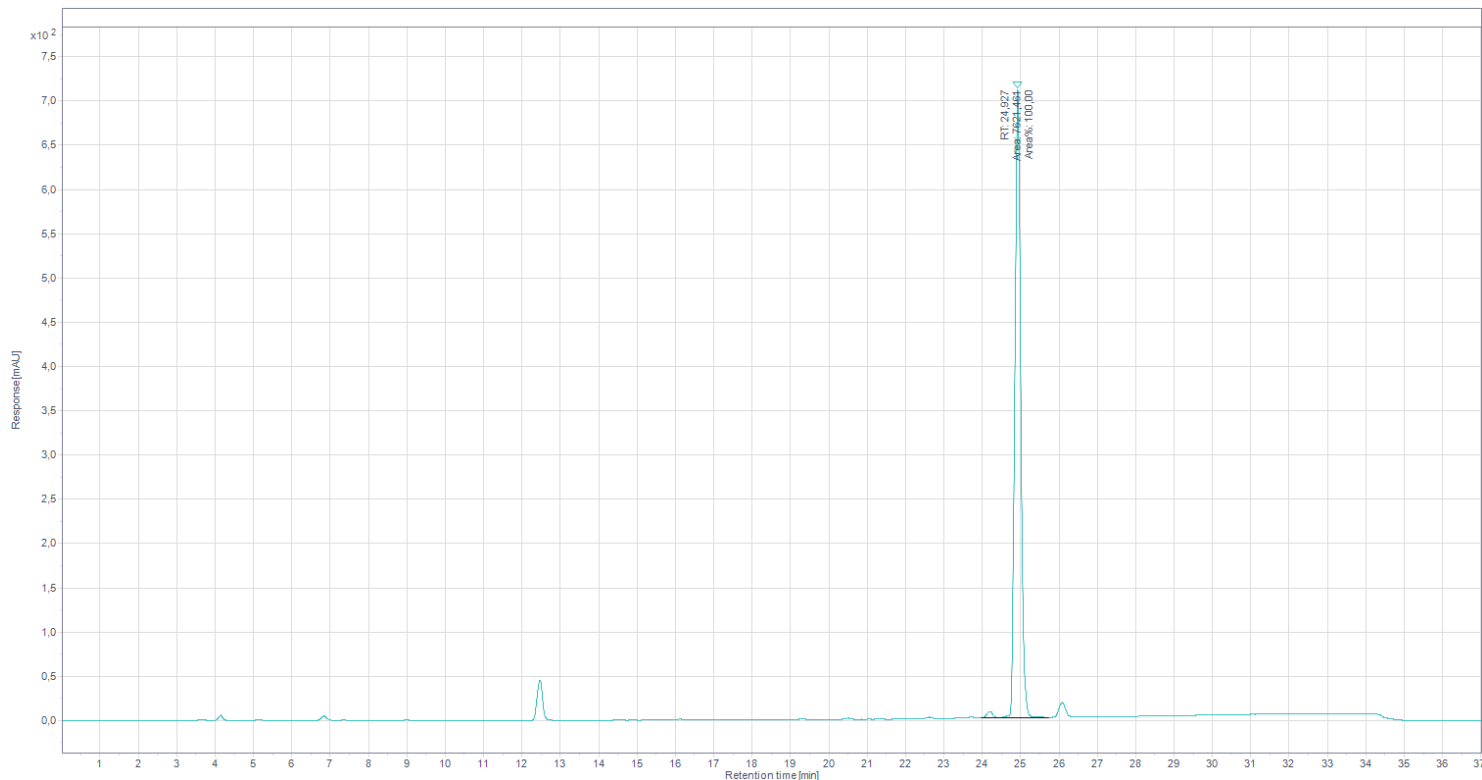

Method

Time	H2O + 0,1% TFA	ACN + 0,1% TFA
0min	60%	40%
2min	60%	40%
27min	5%	95%
30min	5%	95%

Password

A7DB3E9D

Analiza Białek sp. z o.o.

KRS: 0000966168

NIP: 8992922970

REGON: 521751875

Headquarters and Laboratory:

ul. Duńska 9, 54-427 Wrocław

Budynek DELTA

Lab technician:

Analysis and research specialist

mgr Arkadiusz Zajac